



Certificate of Analysis

AHK Copper 100mg

copper (2S)-6-amino-2-[[[(2S)-2-[(2S)-2-aminopropanoyl]azanidyl-3-(1H-imidazol-4-yl)propanoyl]amino]hexanoate


Compound : AHK-Cu
Lot number : NL-213
Analysis date : 2026-08-14
Purity % : 97.57%
Quantity : 117.50 mg
Method : HPLC-UV-MS

Client : Biostrategix
<https://biostrategix.com/>

PubChem CID: 176418766

<https://pubchem.ncbi.nlm.nih.gov/compound/176418766>

High Performance Liquid Chromatography (HPLC) UV – Purity Test

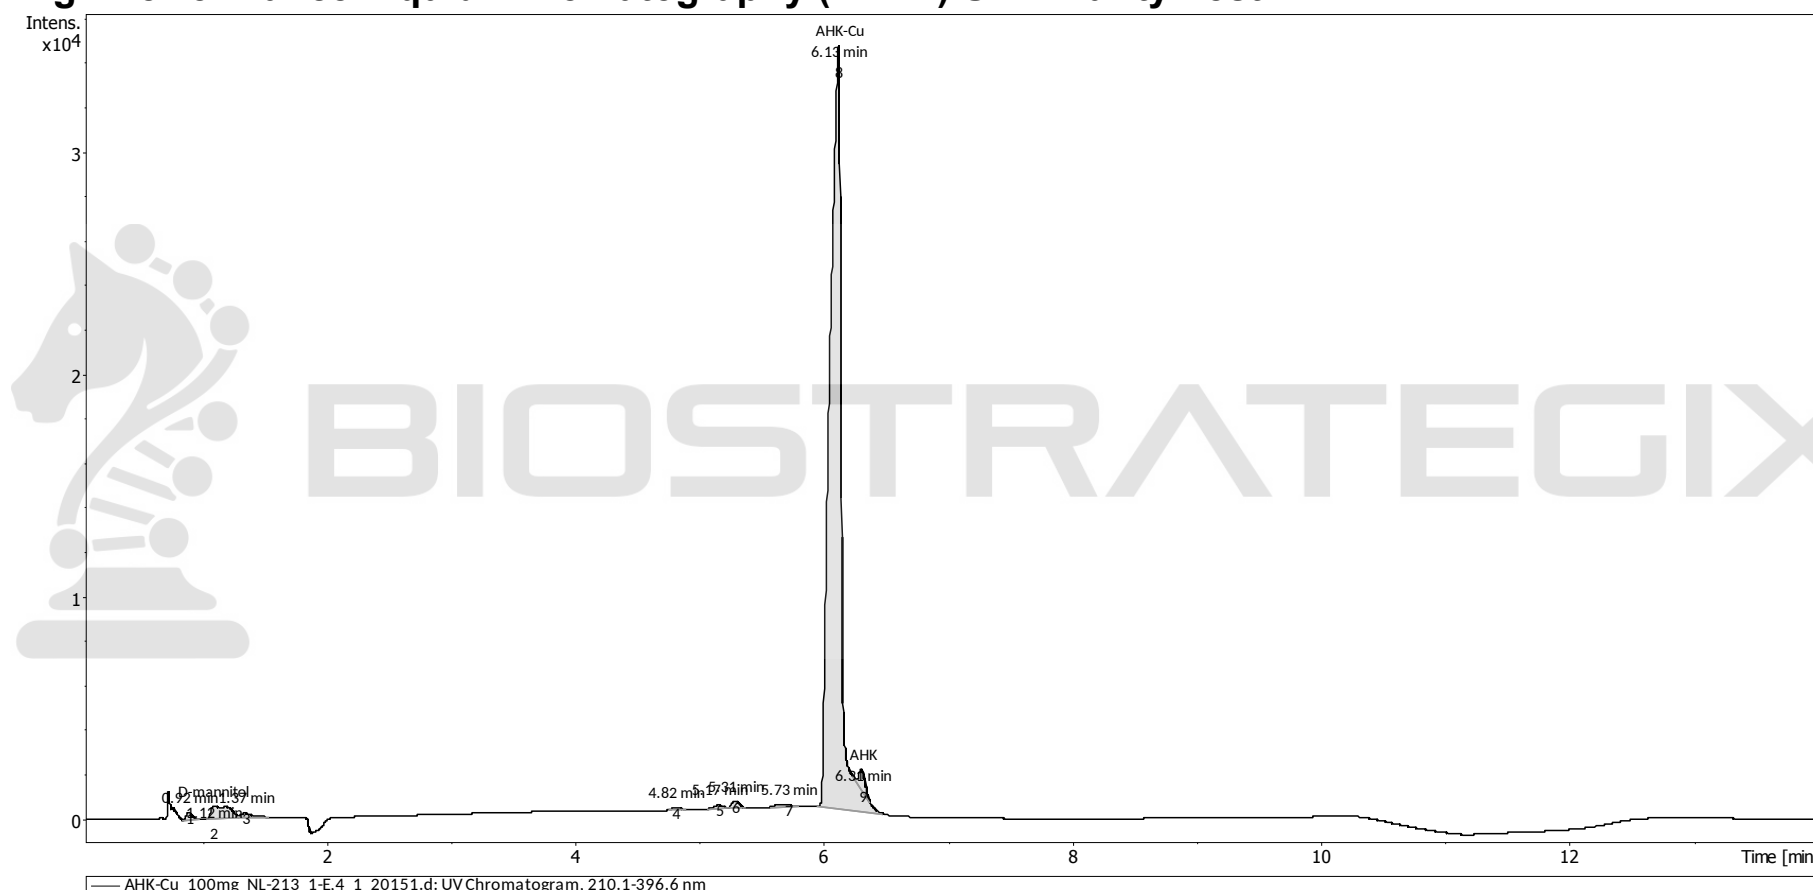

PEAK LIST		Number of detected peaks: 9		
	Time (min)	Area	%Area	
1	0.92	1.12E+03	0.47	
2	1.12	5.96E+03	2.48	D-mannitol
3	1.37	1.45E+03	0.60	
4	4.82	6.03E+02	0.25	
5	5.17	6.15E+02	0.26	
6	5.31	1.15E+03	0.48	
7	5.73	8.90E+02	0.37	
8	6.13	2.25E+05	93.75	AHK Cu
9	6.31	3.23E+03	1.34	AHK

Overall purity : 97.57

Quantification by HPLC-UV

Measured quantity : 117.50 mg/vial

The AHK-Copper complex dissociates slightly during HPLC resulting in the small AHK peak immediately after AHK-Cu. This is normal.

Note: Injectable peptides may contain salts and sugars to aid in solubility and act as pH buffers. These are not normally detected using UV and are not considered impurities.

Analysis Performed by
Ken Pendarvis, ChE
Analytical Chemist
MZ Biolabs
contact@mzbiolabs.com



2026-08-26

AHK Copper 100mg

copper (2S)-6-amino-2-[[[(2S)-2-[(2S)-2-aminopropanoyl]azanidyl-3-(1H-imidazol-4-yl)propanoyl]amino]hexanoate

PubChem CID: 176418766

<https://pubchem.ncbi.nlm.nih.gov/compound/176418766>

Mass Spectrometry (MS) – Identity Test

Identity confirmed using HPLC-MS

Molecular weight calculated using monoisotopic m/z values from mass spectrum

Expected monoisotopic mass : 415.12 Da


Measured monoisotopic mass : 415.14 Da

Molecular weight confirmed

Note : Monoisotopic m/z values are not easily seen in full spectrum view for larger molecules and peptides.

The dominant isotopic peak (base peak) shown in the spectrum below can be used to approximate the average molecular weight frequently reported by vendors and databases as a secondary means of confirmation.

Recorded MS spectrum

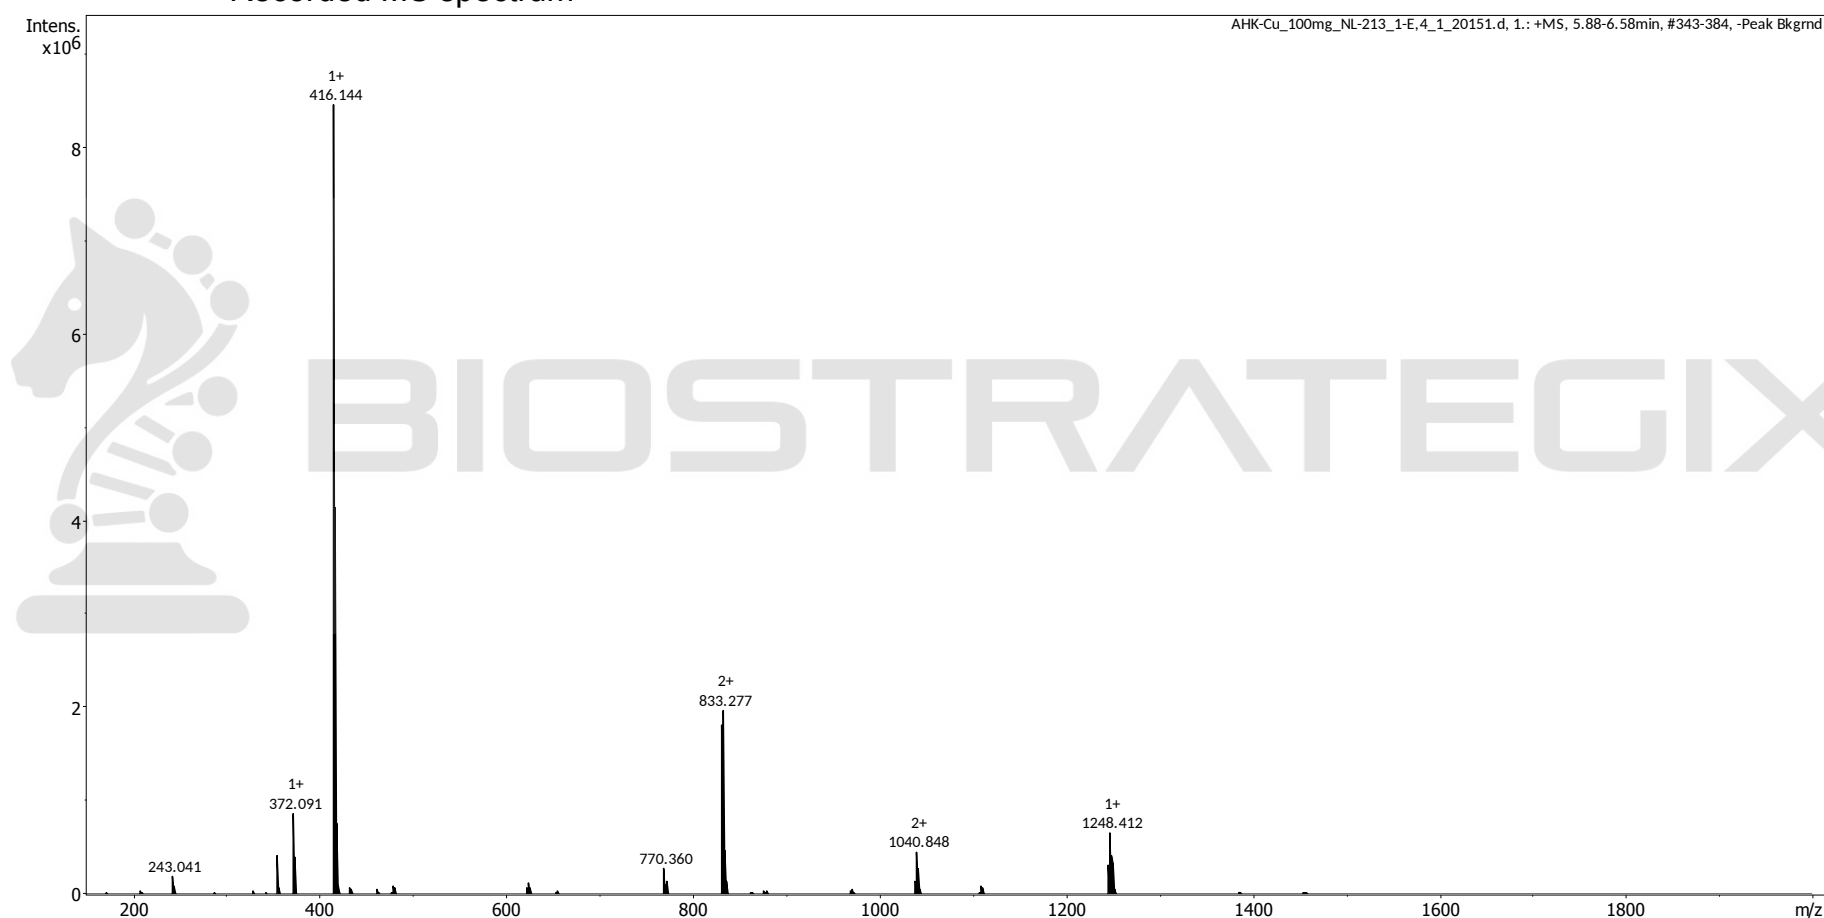

Analysis Performed by
Ken Pendarvis, ChE
Analytical Chemist
MZ Biolabs
contact@mzbiolabs.com



2026-08-26